


1/9

FIG. 1

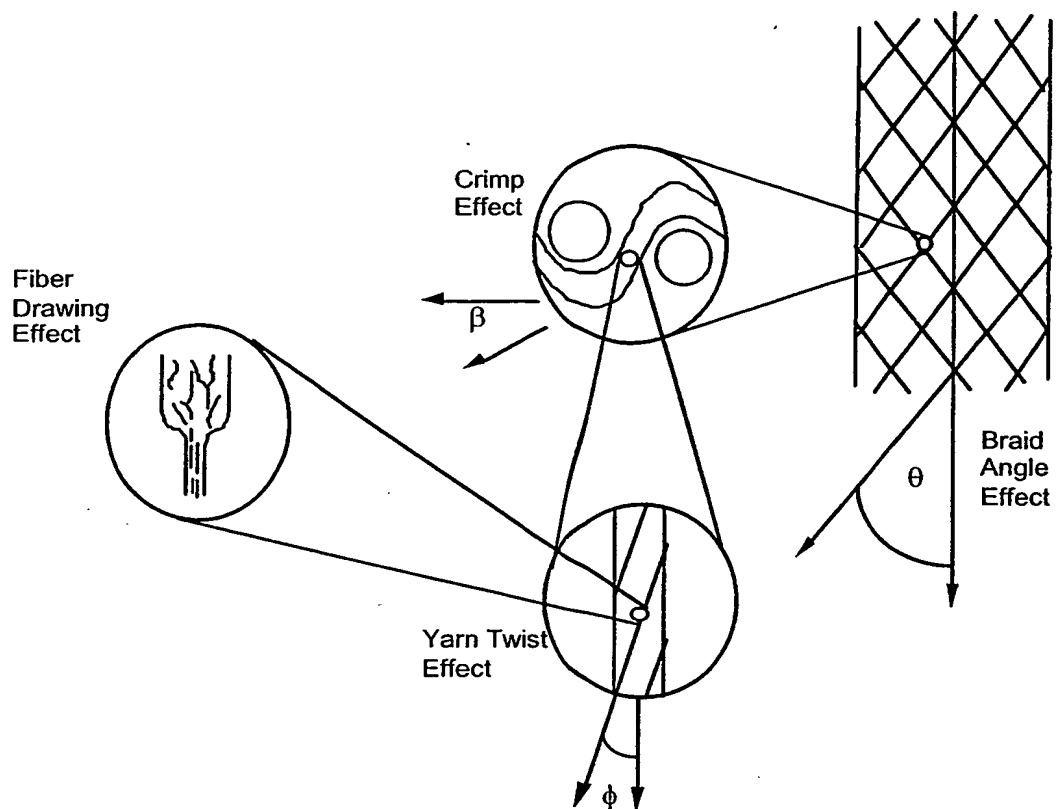

2/9

FIG. 2


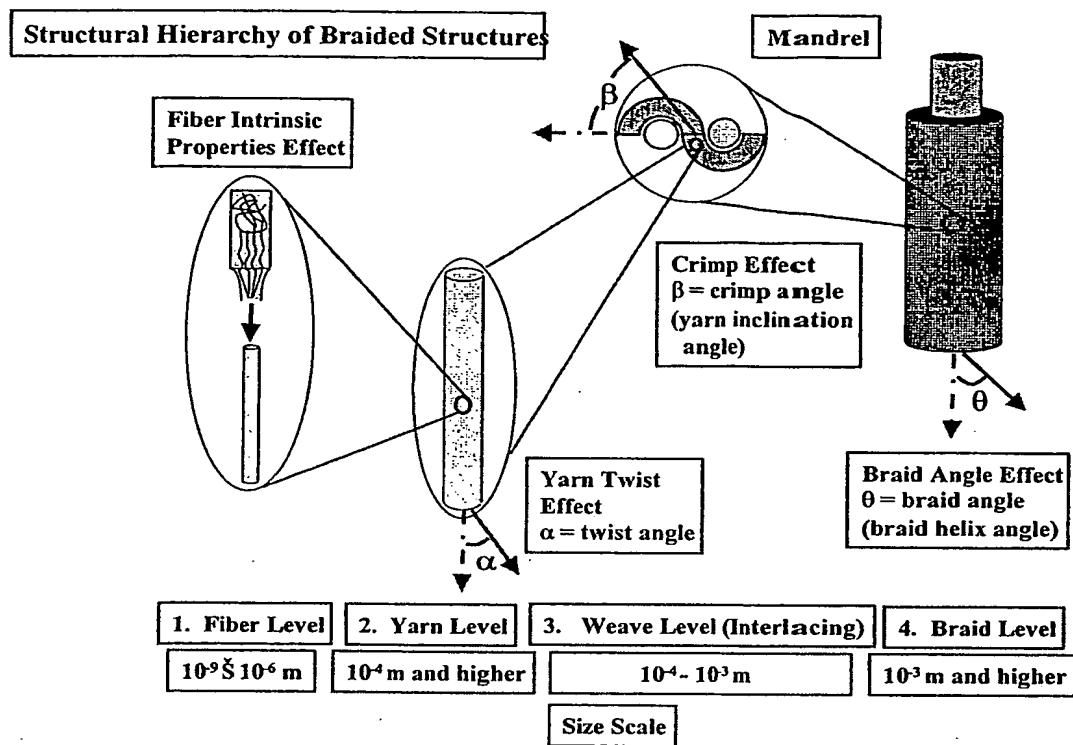


FIG. 3

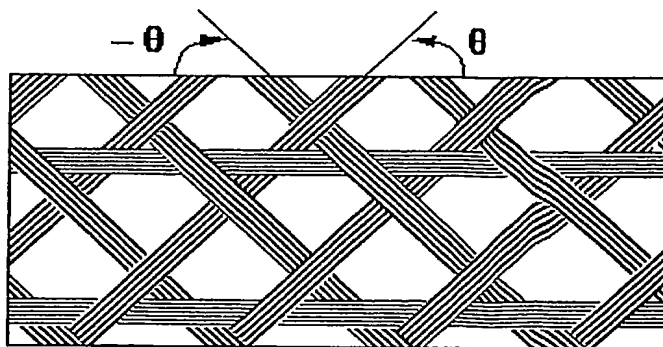

BEST AVAILABLE COPY

3/9

FIG. 4


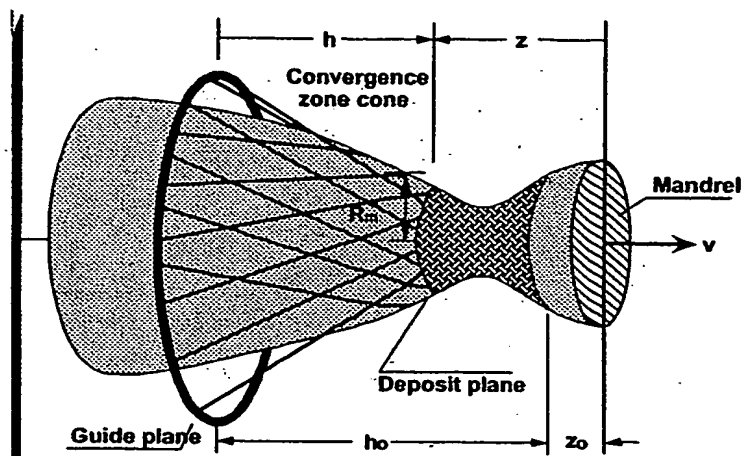


FIG. 5

Process window of fiber volume fraction for braided stent.

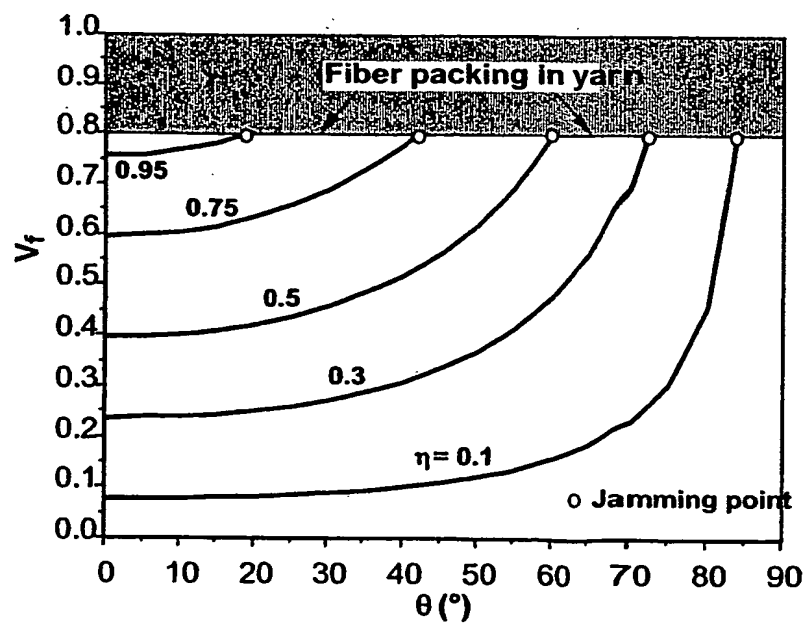


BEST AVAILABLE COPY

FIG. 6A

FIG. 6B

**FIG. 6C**

FIG. 6D

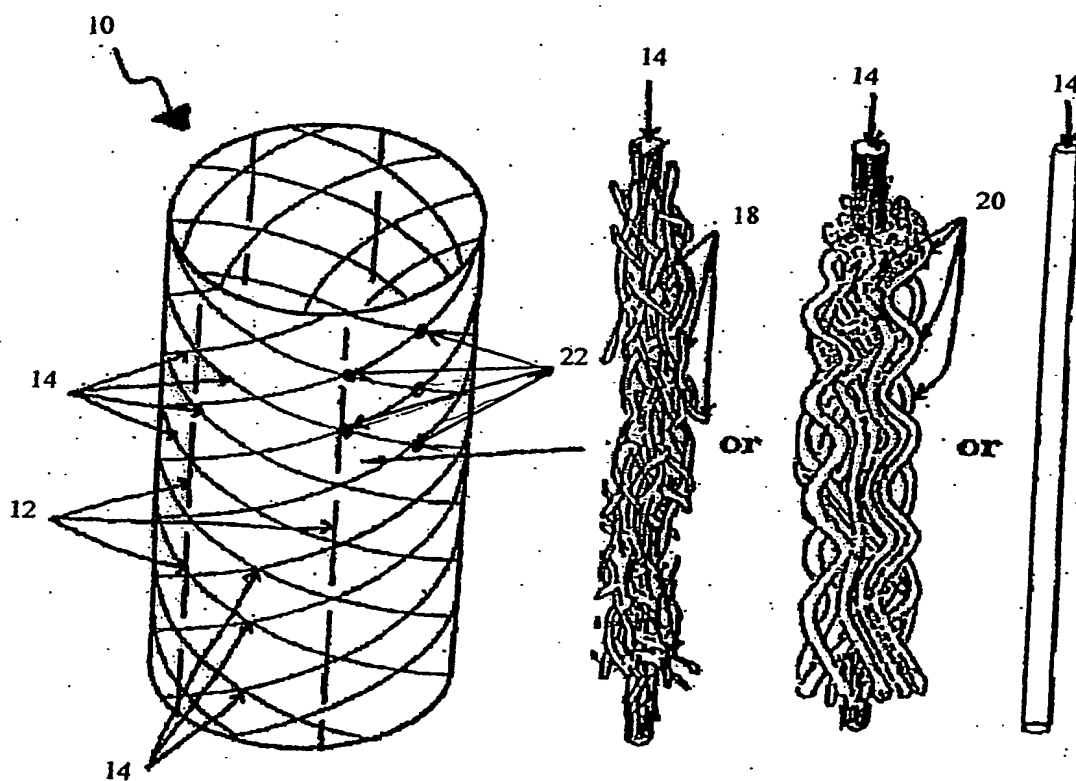

**BEST AVAILABLE COPY**

5/9

FIG. 7A


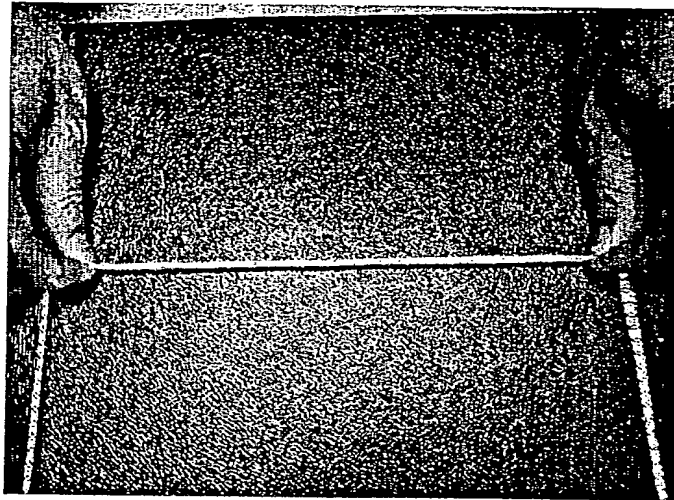



FIG 7B

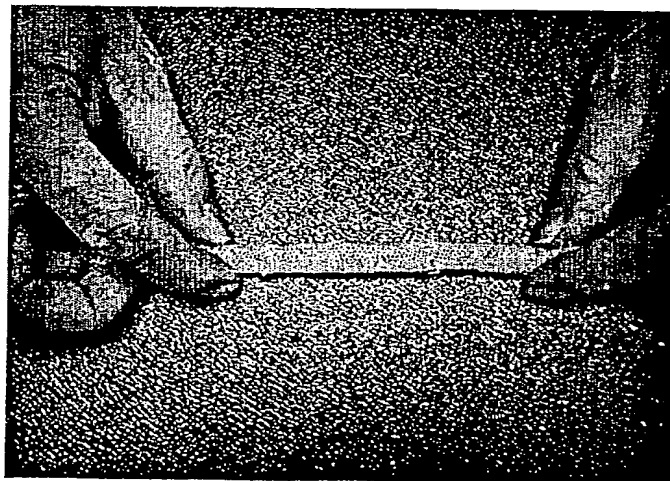

BEST AVAILABLE COPY

6/9

FIG. 8

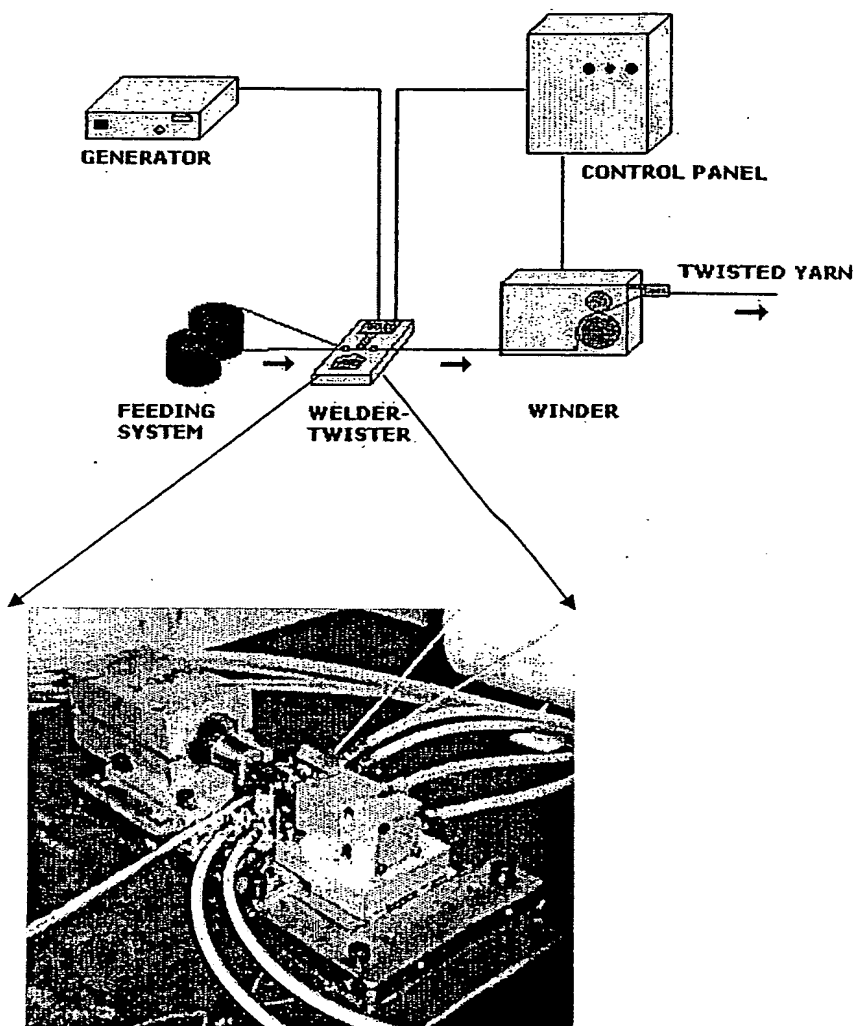

BEST AVAILABLE COPY

7/9

FIG. 9A


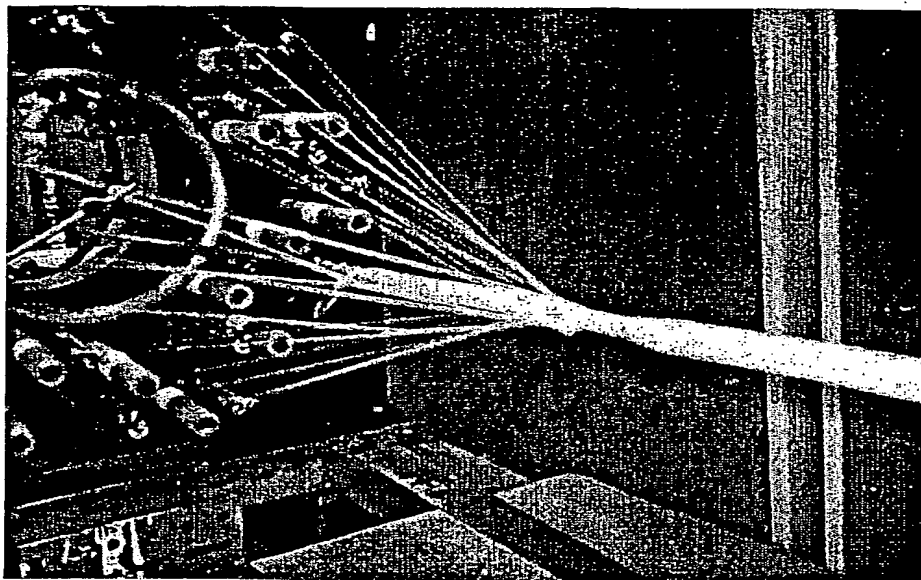



FIG. 9B

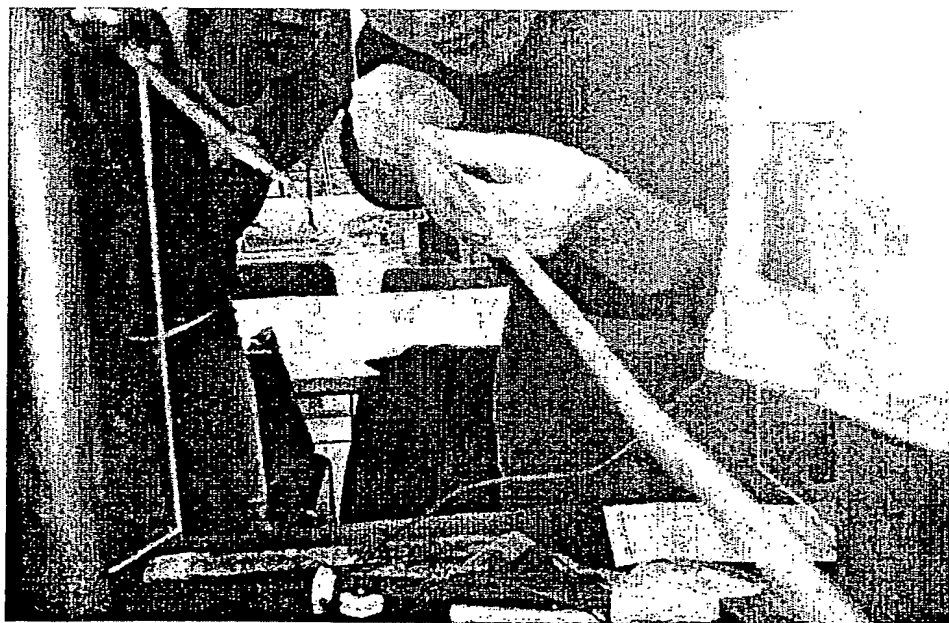

BEST AVAILABLE COPY

8/9

FIG. 10

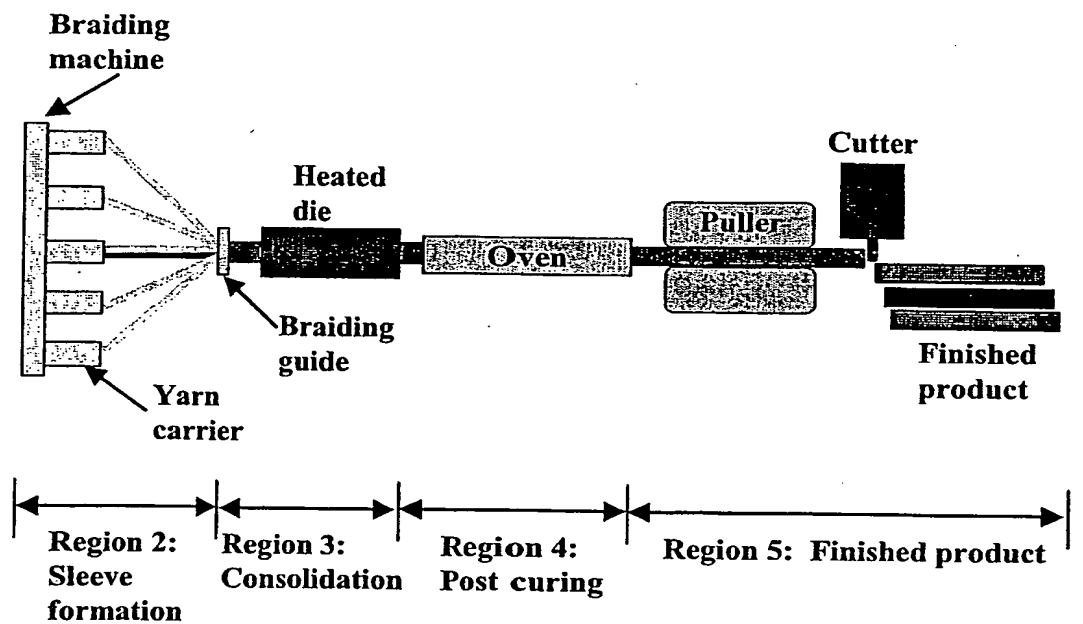

BEST AVAILABLE COPY



9/9

FIG. 11

